

Tension Meter

**SCHMIDT**  
control instruments




Edition DX 01.2.E

DX Series

Model DXK

# Instruction Manual

Valid as of: 01.03.2008 • Please keep the manual for future reference!

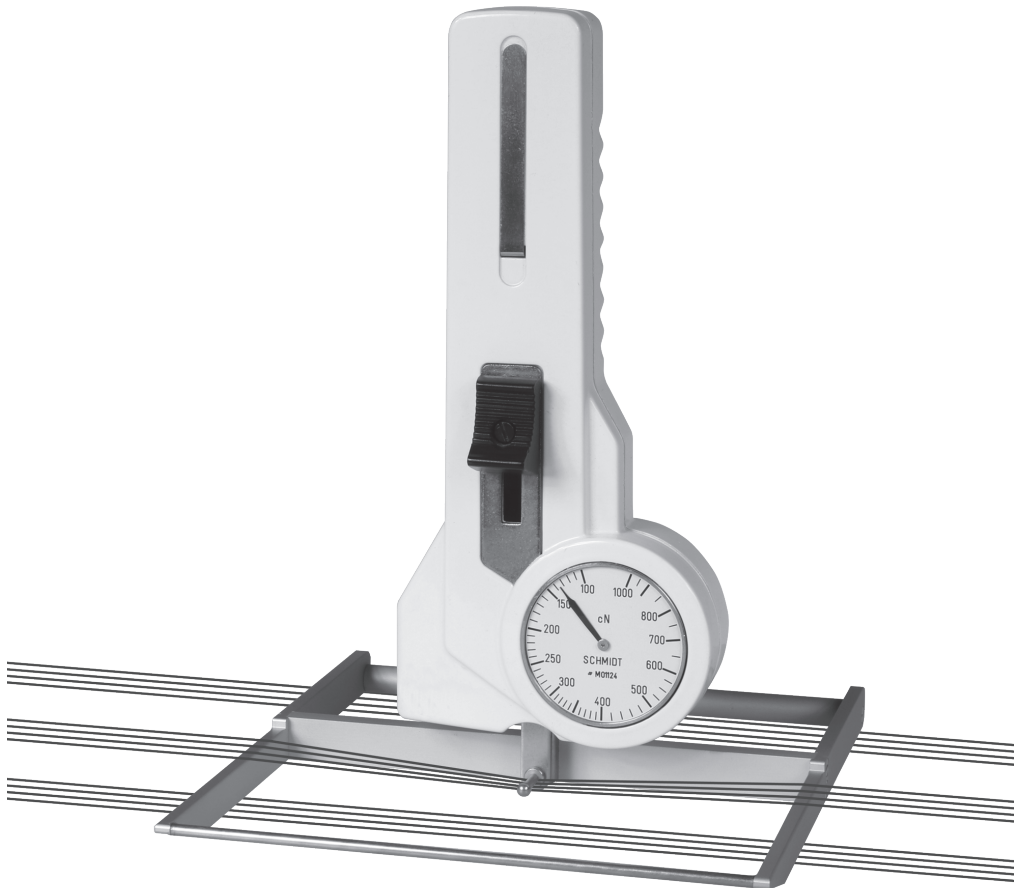

**SCHMIDT** · 1<sup>ST</sup> IN TENSIONMETERS WORLDWIDE

# Contents

<b>1 Warranty and liability</b> .....	<b>3</b>
1.1 Notices within the instruction manual .....	3
1.2 Responsibilities of the operating company .....	3
1.3 Responsibilities of the personnel .....	3
1.4 Informal safety measures .....	4
1.5 Training of the personnel .....	4
1.6 Intended use .....	4
1.7 Dangers in handling the device .....	4
1.8 Copyright .....	4
1.9 Declaration of conformity .....	4
<b>2 Available models</b> .....	<b>5</b>
2.1 Specifications .....	5
2.2 Optional accessories .....	5
2.3 Delivery includes .....	5
2.4 Unpacking .....	5
<b>3 Measuring</b> .....	<b>6</b>
3.1 Notices before starting measurement .....	6
3.1.1 Mounting the special finger support (on the rear side of the tension meter) ..	6
3.2 Measuring with the tension meter .....	7
3.3 Memory pointer (optional accessory Code M) .....	8
<b>4 Service and maintenance</b> .....	<b>9</b>
<b>5 Cleaning</b> .....	<b>9</b>
<b>6 Verification intervals</b> .....	<b>9</b>
6.1 Verification of calibration and determination of repair costs .....	10
<b>7 Correspondence</b> .....	<b>11</b>
<b>8 Repairs</b> .....	<b>11</b>

## 1 Warranty and liability

In principle, the supply of the device is subject to our “General Conditions of Sale and Delivery.” These have been provided to the operating company on conclusion of the contract, at the latest.

Warranty:

- SCHMIDT tension meters are warranted for 12 months.

Parts subject to wear, electronic components and measuring springs are not covered by the warranty. No warranty or liability will be accepted for bodily injury or property damage resulting from one or several of the following causes:

- Misuse or abuse of the device.
- Improper mounting, commissioning, operation and maintenance of the device (e.g. verification interval).
- Operation of the device if any safeguards are defective or if any safety and protection precautions are not properly installed or not operative.
- Failure to comply with the notices in the instruction manual regarding transport, storage, mounting, commissioning, operation, maintenance and setup of the device.
- Any unauthorized structural alteration of the device.
- Insufficient inspection of device components that are subject to wear.
- Opening the device or improper repair work.
- Disasters caused by the effects of foreign objects or by force majeure.

### 1.1 Notices within the instruction manual

The fundamental prerequisite for the safe handling of this device and its troublefree operation is the knowledge of the basic safety notices and safety instructions.

This instruction manual contains the most important notices for the safe operation of the device.

These instruction manual, in particular the safety notices, must be observed by any person who works with the device. In addition, the local valid rules and regulations for the prevention of accidents must be complied with.

The representations within the instruction manual are not true to scale.

The dimensions given are not binding.

General indications of direction, such as FRONT, REAR, RIGHT, LEFT apply when viewing the front of the device.

### 1.2 Responsibilities of the operating company

In compliance with the EC Directive 89/655/EEC, the operating company agrees to only permit persons to work with the device who:

- are familiar with the basic regulations on industrial safety and accident prevention and who have been trained in handling the device.
- have read and understood the chapter on safety and the warning notices in these instruction manual and have confirmed this with their signatures.
- are examined regularly on their safe and conscientious working method.

### 1.3 Responsibilities of the personnel

All persons who work with the device agree to perform the following duties before starting work:

- to observe the basic regulations on industrial safety and accident prevention.
- to read the chapter on safety and the warning notices in these instruction manual and to confirm with their signatures that they have understood them.

## 1.4 Informal safety measures

The instruction manual must always be kept on hand where the device is operated. Apart from the instruction manual, the generally and locally valid regulations on accident prevention and environmental protection must be provided and complied with.

## 1.5 Training of the personnel

Only trained and instructed personnel is permitted to work with the device. The responsibilities of the personnel must be clearly defined for mounting, commissioning, operation, setup, maintenance and repair. Trainees may only work with the device under the supervision of an experienced personnel

## 1.6 Intended use

The device is intended exclusively to be used as a tension meter. Any other use or any use exceeding this intention will be regarded as misuse. Under no circumstances shall Hans Schmidt & Co GmbH be held liable for damage resulting from misuse.

The intended use also includes:

- Complying with all notices included in the instruction manual and observing all inspection and maintenance works.

## 1.7 Dangers in handling the device

The device was designed according to the state of the art and the approved safety standards. Nevertheless, its use may cause serious or fatal injury to the user or third persons, and/or an impairment of the device or of other material assets.

The device may only be applied:

- For its intended use in a faultless condition with regard to the safety requirements.
- Malfunctions that could impair safety must be remedied immediately.
- Personal protective equipment must be used according to the EC Directive 89/686/EEC.



**The device must not be operated in potential explosive areas and must not come into contact with aggressive substances.**

## 1.8 Copyright

The copyright on these instruction manual remains with the company Hans Schmidt & Co GmbH.

These instruction manual are intended for the operating company and its personnel only. They contain instructions and notices that may only be reproduced on the prior written permission of

Hans Schmidt & Co GmbH

and under indication of the complete reference data.

Violations will be prosecuted.

## 1.9 Declaration of conformity

Our mechanical tension meters do not belong to the EC machinery directive 2006/42/EG and do not have a CE mark.

## 2 Available models

Model	Tension Range cN	Reference Frame cm
DXK-300	20 - 300	15 x 17
DXK-1000	100 - 1000	15 x 17
DXK-2000	200 - 2000	15 x 17

SCHMIDT calibration with fabric tape

Other tension ranges available on request

Other units of measure available, such as g

International unit for tension force: 1 cN = 1.02 g = 0.01 N

1 daN = 1.02 kg = 10.0 N

### 2.1 Specifications

**Calibration:** According to SCHMIDT factory procedure

**Accuracy:** ± 1% full scale or ± 1 graduation on scale

**Sensing pin width:** 10 mm (option 34 mm)

**Scale diameter:** 41 mm

**Temperature range:** 10 - 45°C

**Air humidity:** 85% RH, max.

**Housing material:** Die-cast aluminium

**Housing dimensions**

(without measuring frame): 188 x 85 x 45 mm (L x W x H)

**Weight net (gross):** Approx. 470 g (1000 g)

### 2.2 Optional accessories

Code M: Memory pointer

### 2.3 Delivery includes

- Tension meter
- Special finger support
- Certificate of Compliance with the order 2.1 under EN 10204
- Instruction manual
- Carrying case

### 2.4 Unpacking

Unpack the tension meter and inspect it for any shipping damage.

Notices of defect must be announced immediately, at the latest within 7 days on receipt of the goods.

### 3 Measuring

#### 3.1 Notices before starting measurement




Have you read and understood the instruction manual, in particular chapter 1 “Warranty and liability” ?

You are not permitted to operate the device before doing so.

Before working with the device you must put on your personal protective clothing, if necessary. For example, eye protectors, gloves, etc. To avoid damage, do not move the measuring feeler by hand.


Tensions that exceed the tension range of the instrument by more than 100 % may cause permanent damage to the movement and must be avoided under any circumstances.

- 1 The ID plate with the serial number as well as the calibration label (optional) are provided on the bottom of the instrument, the SCHMIDT quality seal are provided on the surface.

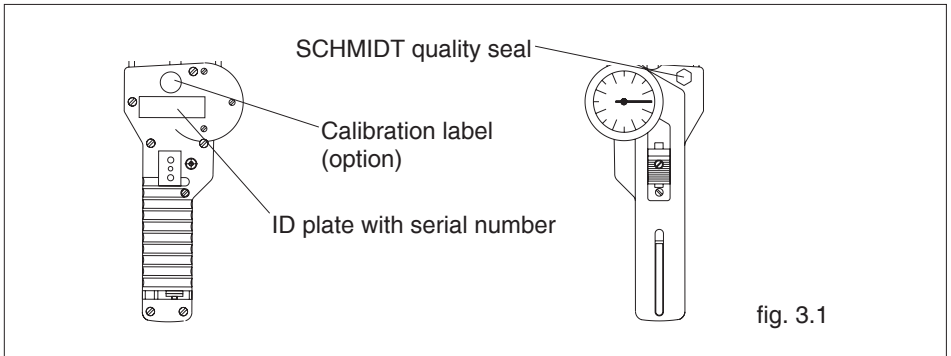

#### 3.1.1 Mounting the special finger support (on the rear side of the tension meter)


Whenever useful and necessary, the tension meter is supplied with a special finger support when measuring high tensions (with Model DXK-1000 and higher tension ranges) to reduce the necessary effort to move the outer rollers with the Thumb piece on the front of the tension meter and facilitate acquisition of the material to be measured. (chapter 3.2)

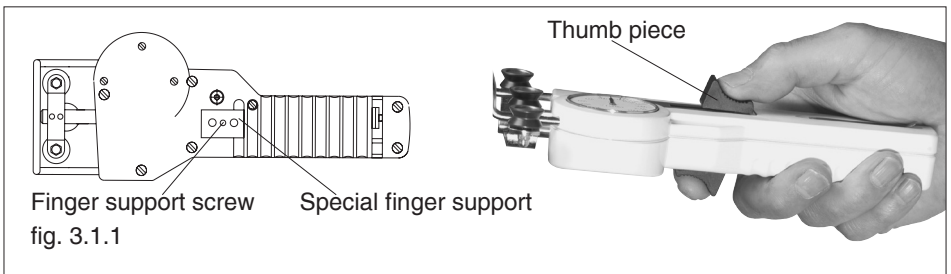


- Place the special finger support in the recess located on the rear side of the tension meter and fasten it with the finger support screw.

## 3.2 Measuring with the tension meter

### Inserting

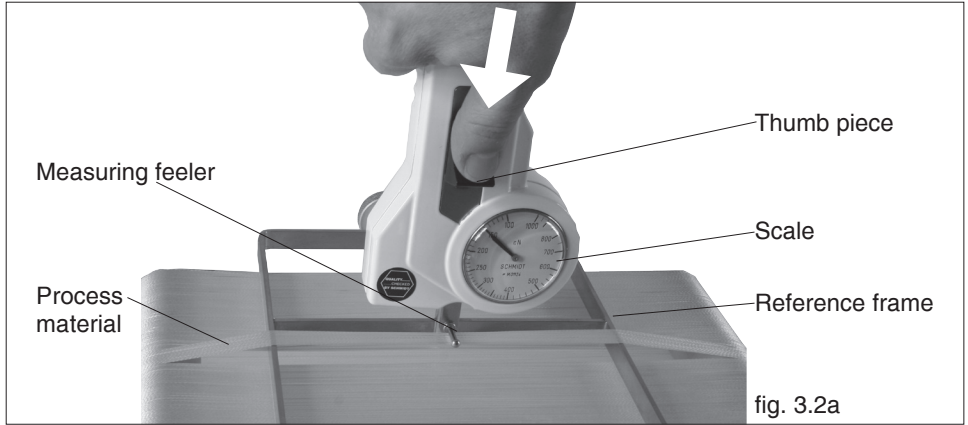

### Measuring position

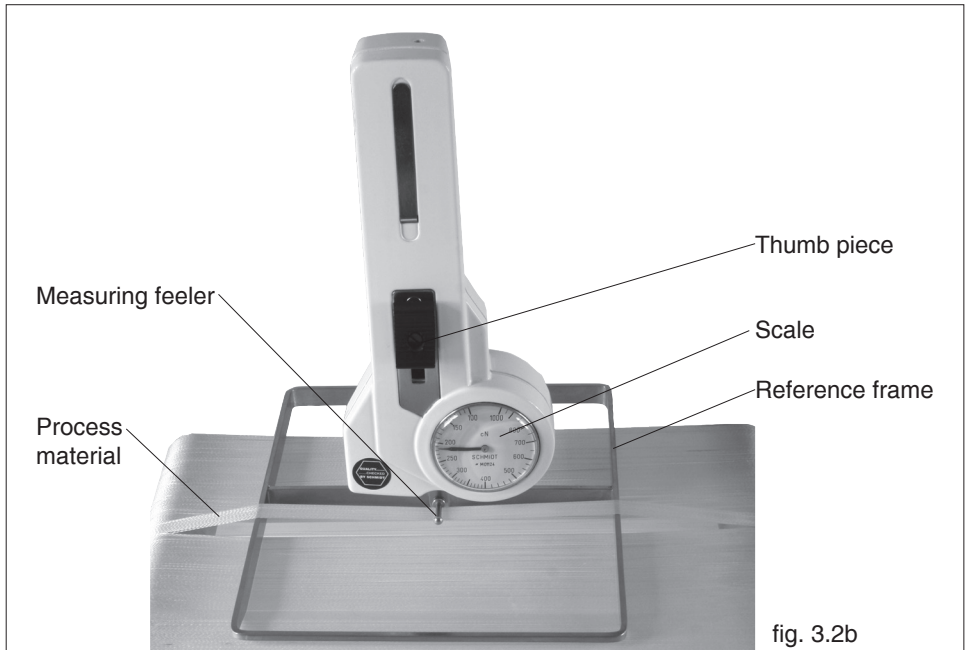

### 3.2 Measuring with the tension meter (cont.)

#### General information:

We recommend always measuring the same number of ends, such as 5 or 10 ends (repeat of pattern) or only a single end at a time.

#### Requirements:

The weaving machine is not running.

#### Inserting:

- Push the thumb piece as far as it will go in the direction of the arrow to extend the reference frame.
- The reference frame must abut on the process material. (fig. 3.2a).
- **Slowly** release pressure on the thumb piece until the Reference frame return to his original position.

It is important to assure that the process material runs smoothly between the roller guides and the measuring roller.



**It is essential that the thumb piece return slowly to its initial position. Any uncontrolled snap-back may affect calibration and may also damage the instrument.**

- Set the tension meter with the reference frame down on the warp threads.
- Unhand the tension meter (fig. 3.2b).  
The scale pointer will now show the line tension directly.



**During the measuring the process material has to stay in the same position**

#### Removing:

- Push the thumb piece as far as it will go in the direction of the arrow.
- With the reference frame extended, move the instrument away from the material.
- Slowly release pressure on the Thumb piece until the outer rollers return to their original position.


### 3.3 Memory pointer (optional accessory Code M)

The tension meter Model DXK can be factory-equipped with a memory pointer for retaining the highest reading obtained during a measuring period.

This is achieved by a memory pointer which trails the scale pointer and stops at the highest tension reading (Peak value) obtained during the measuring period.

#### To reset the memory pointer before a new measuring period:

- Set the memory pointer to zero manually with the knurled screw.

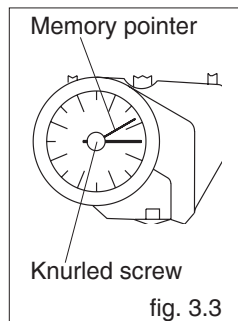

#### 4 Service and maintenance

The tension meter is easy to maintain.

Depending on operating time and load, the tension meter should be checked according to the locally valid regulations and conditions.

#### 5 Cleaning

For cleaning the unit, do not use any



##### **AGGRESSIVE SOLVENTS**

such as trichloroethylene or similar chemicals.



##### **NO WARRANTY OR LIABILITY**

shall be accepted for damage resulting from improper cleaning.

#### 6 Verification intervals

The question of finding the right frequency of calibration accuracy verification depends on several different factors:


- Operating time and load of the SCHMIDT tension meter
- Tolerance band defined by the customer
- Changes of the tolerance band compared to previous verifications of calibration

Therefore, the interval between verifications must be determined by the user's Quality Assurance Department based on the user's experience.

Assuming normal operating time and load as well as careful handling of the tension meter, we recommend a verification interval of 1 year.

## 6.1 Verification of calibration and determination of repair costs

Flow chart for verifying the calibration of used tension meters, incoming and outgoing verification with Inspection Certificate 3.1 according to DIN EN 10204

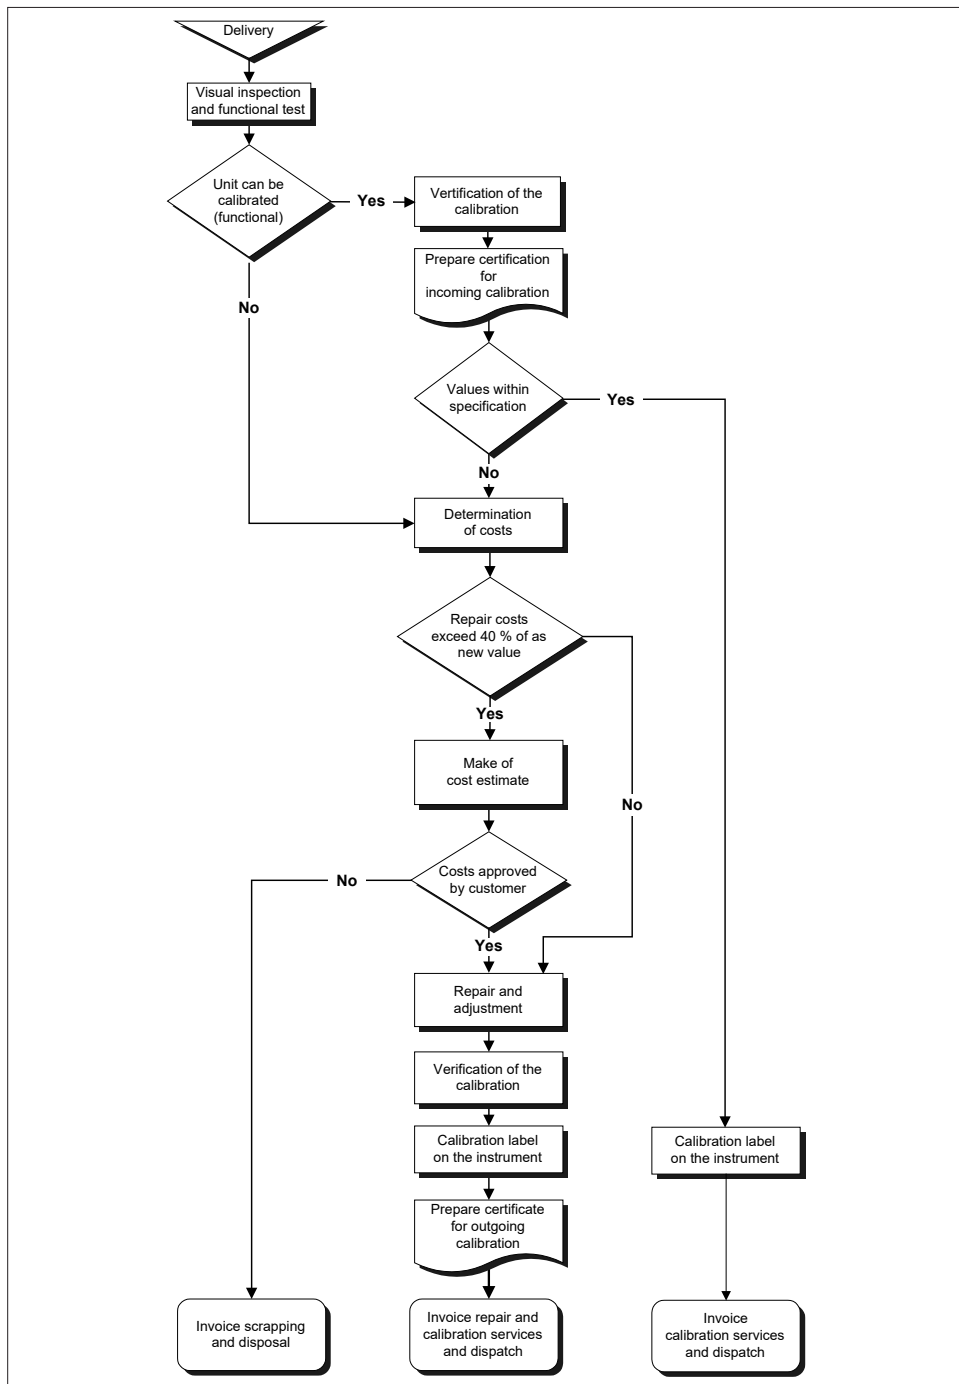

## 7 Correspondence

Should you have any questions regarding the instrument or instruction manual, or their use, please indicate above all the following details which are given on the ID plate:

- 1) Model
- 2) Serial number

## 8 Repairs

### Shipping instructions:

We kindly ask for return free of charge for us, if possible by airmail parcel. All occurring charges, if any (such as freight, customs clearance, duty etc.), will be billed to customer. For return from foreign countries, we ask you to include a proforma invoice with a low value for customs clearance only, e.g. 50 Euro, each and to advise the shipment in advance by fax or eMail.



**To avoid unnecessary follow-up questions, and the resulting loss of time or possible misunderstandings, please return the instrument with a detailed fault description to our service department. Please indicate in your order whether you require an Inspection Certificate 3.1 according to DIN EN 10204.**

Service address:

**Hans Schmidt & Co GmbH  
Schichtstr. 16  
D-84478 Waldkraiburg  
Germany**

Notes:

---

---

**SCHMIDT**

control instruments

**SCHMIDT-Test-Instruments**  
indispensable in production monitoring,  
quality control and automation  
We solve your measuring problems:



Tension Meter



Force Gauge



Torque Meter



Tachometer



Speed- and Lengthmeter



Electronic Lengthmeter



Stroboscope



Screen Printing Tension Meter



Thickness Gauge



Yarn Package Durometer and Shore Durometer



Sample Cutter



Balance



Moisture Meter



Leak Tester

**More than 75 years - Worldwide -**

**Hans Schmidt & Co GmbH**

**Mailing address:**

P. O. B. 1154  
84464 Waldkraiburg Germany

**Shipping address:**

Schichtstr. 16  
84478 Waldkraiburg Germany

**Phone:**

int. + 49 / (0)8638 / 9410-0

**Fax:**

int. + 49 / (0)8638 / 4825

int. + 49 / (0)8638 / 67898

**e-mail:**

info@hans-schmidt.com

**Internet:**

http://www.hans-schmidt.com